



BAKER GAUGES INDIA PRIVATE LIMITED

CORPORATE OFFICE & FACTORY :

BMI DIVISION

33-1-2, NAGAR ROAD, PUNE 411 014, INDIA

TEL.: (020) 66093800

E-mail : bakerbmi@bakergauges.com * www.bakergauges.com

BAKER

...a passion for precision

Calibration Certificate

TRUE COPY

ULR -CC276425000001506F	Date of Issue : 12.09.2025
Calibration Certificate No.: LAB/CA/01/02/25/1506	Date of Calibration n: 12.09.2025
Date of receipt: 05.09.2025	Page 1 of 1
Customer Name & Address: NCQC Laboratory LLP House No. 4, Abhishree Corporate Park, Nr. Swagat Bungalow BRTS, Iskcon-Ambli Road, Ambli, Ahmedabad - 380 058.	Customer Reference no.: Delivery Challan No. 01092025/05 dtd. 01.09.2025
Description of Item: OD Master (Master Setting Disc)	Our Reference No.: CA 001347 dtd 05.09.2025
	Calibration Procedure No: LAB/WI/04
	Environmental Condition: Temperature: 20°±1°C

Received Condition of Item: Visually OK

Equipments/Masters used for Calibration:

Master/Equipment	Sr. No.	Certificate No.	Valid upto
Sigma Comparator	EC-449	25021576/D1.02/C-025	April 2027
Gauge Block Set	230003	RCL23/12/212/002	Dec. 2025

Mechanical Calibration:

Calibration Results:

Item No.	Sr. No. / Id. No. Make	Etched Size (mm)	Actual Size (mm)	Remarks	Uncertainty of Measurement (µm)
1	G3640 Octagon	125.0025	125.0030	Taper 0.5 µm Ovality 0.5 µm	±1.10


Note - Next date of calibration (As Required by Customer) 12.09.2027

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=1.96 such that coverage probability corresponds to 95 %.

NCQC System Certificate No. 228/1

For Baker Gauges India Pvt. Ltd. (BMI Div.)

S. L. Vishwakarma
Calibrated by
Engineer - Standard Room
(S.L. Vishwakarma)

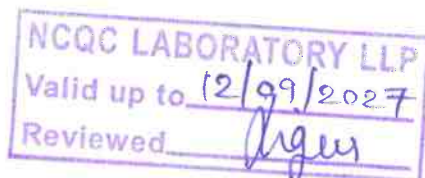

[Signature]
Approved by
Technical Manager-Standard Room
(A. V. Alloli)