



CC-2743

Format No.: 7.8-QF-02

D - 46, Sector - 4, DSIIIDC, Bawana, Delhi - 110 039, INDIA
Phone : +91-11-47092663 E-mail : info@weightronics.net**Calibration Certificate**


Issue Dated: 10-01-2022

Recommended Date for the Next Calibration Mentioned As Per Request of the Customer	Page	No. of Pages
Date: 07-01-2024	-1-	-2-

Certificate No.: WMCL/E/2022-01/1632/amend
ULR - CC274322000001632F

Date of Calibration: 08-01-2022

Calibrated for	:	NATIONAL CENTRE FOR QUALITY CALIBRATION 4, Abhishree Corporate Park, Near Swagat Bunglow BRTS, Iskcon-Ambli Road, Ambli, Ahmedabad - 380 058, Gujarat, INDIA
Customer Reference	:	RGP No.: 21122021, Dated: 21/12/2021
Service Request No	:	7.1-QF-01-1632
Date of Receipt	:	23/12/2021
Condition of Receipt	:	Non Satisfactorily
Calibrated at	:	Laboratory
Description of Instrument	:	Make - "WEIGHTRONICS"
10 kg, 5 kg	:	Stainless Steel Knob Type Cylindrical Weights
Manufacturer Serial No	:	---
Customer Identification No	:	---
Assumed Density (d)	:	(7 950 ± 140) kg/m ³ ; (k=2) for Stainless Steel
Environmental Conditions	:	Temperature : (23.0 ± 2.0)°C Relative Humidity : (50.0 ± 10.0) % [Change in Temperature and Relative Humidity during the calibration were less than ± 0.7°C per hour and ± 10.0 % per 4 hours respectively]
Standard (s) used	:	WMCL working standard of mass with uncertainty Better than one-third of the reported uncertainty of measurement
Traceability Standard (s)	:	The Standard used for Calibration are Traceable from "NPL" New Delhi, INDIA vide Calibration Certificate No.: 19100740/D1.01/C-114, Dated: 03/12/2019 valid up to Dated: 03/12/2022
Balance used for Calibration	:	Precision Balances of Appropriate Accuracy Traceable to Mass Standards
Methodology of Calibration Adopted	:	The Method of comparison with standard (s) using Substitution Weighing Method and (ABBA or ABA) Weighing Cycle, The Reported Mass Values(s) is (are) the conventional mass value(s) (M _C) related to the true mass value(s) (M _T) by formula: M _C =M _T [1-1.2(1/d-1/8000)]. (Where, 'd' is in kg/m ³). (Cal. Procedure No.: WMCL-CP-01)

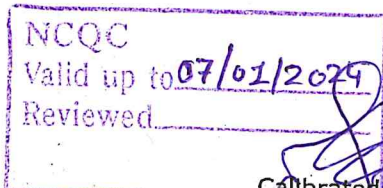

Calibrated by:

Bharat Bhushan



Issued by:

Lalit Shukla
Authorized Signatory

NCQC System Certificate No. 145



CC-2743

Format No.: 7.8-QF-02

D - 46, Sector - 4, DSIIDC, Bawana, Delhi - 110 039, INDIA
Phone : +91-11-47092663 E-mail : info@weightronics.net**Calibration Certificate**

Issue Dated: 10-01-2022

Recommended Date for the Next Calibration Mentioned As Per Request of the Customer Date: 07-01-2024	Page -2-	No. of Pages -2-
--	-----------------	-------------------------

Certificate No.: WMCL/E/2022-01/1632/amend
ULR - CC274322000001632F

Date of Calibration: 08-01-20 22

Results:

ID. No.	Denomination	Mass Value (g)	Uncertainty (\pm g)
NCQC/M-52	10 kg	9 999.990	0.005
NCQC/M-53	5 kg	4 999.995	0.002 5

Remarks: Mass Values of all the weights are conventional mass values and within the maximum errors permissible in "E₂" Accuracy Class of Weights as per OIML R 111-1:2004.

The Reported uncertainty is at coverage factor $k=2$ which corresponds to a coverage probability of approximately 95% for a normal distribution. The contribution of uncertainty originating from the standard used, the weighing process, drift in standard and the air buoyancy correction are taken in to account.

Notes: This Calibration Certificate may not be reproduced except in full, unless written Permission for Publication of an approved extract has been obtained from the Laboratory (WMCL).


- The Calibration results reported in this Certificate are valid at the time of and under the stated conditions of measurement.
- The Calibration results refer only to the particular item submitted for calibration.
- The Calibration Certificate issued for Weights, Weighing Balance used for Scientific or Industrial purposes only and not used for Commercial.

This Calibration Certificate is issued on 29/03/2023 in lieu of the earlier Certificate No.: WMCL/E/2022-01/1632, Dated: 08/01/2022.

Calibrated by:


Bharat Bhushan


Issued by:


Lalit Shukla
Authorized Signatory
